

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
9 August 2001 (09.08.2001)

PCT

(10) International Publication Number  
WO 01/56654 A1

(51) International Patent Classification<sup>7</sup>: A61N 1/372,  
A61B 5/00, G06F 17/60

G.; 3720 Wellington Court, Plymouth, MN 55441 (US).  
THOMPSON, David, L.; 14171 Alder Street Northwest,  
Andover, MN 55304 (US).

(21) International Application Number: PCT/US01/03417

(22) International Filing Date: 2 February 2001 (02.02.2001)

(74) Agents: WOLDE-MICHAEL, Girma et al.; Medtronic,  
Inc., MS301, 7000 Central Avenue NE, Minneapolis, MN  
55432 (US).

(25) Filing Language: English

(81) Designated States (national): CA, JP.

(26) Publication Language: English

(30) Priority Data:  
60/180,289 4 February 2000 (04.02.2000) US

(84) Designated States (regional): European patent (AT, BE,  
CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC,  
NL, PT, SE, TR).


(71) Applicant: MEDTRONIC, INC. [US/US]; 7000 Central  
Avenue NE, Minneapolis, MN 55432 (US).

Published:  
— with international search report  
— before the expiration of the time limit for amending the  
claims and to be republished in the event of receipt of  
amendments

(72) Inventors: MCMENIMEN, James, L.; 935 East LaJolla  
Drive, Tempe, AZ 85282 (US). CAMPBELL, Christo-  
pher, J.; 707 Heron Circle North, Oakdale, MN 55128  
(US). RUBLE, Barbara, K.; 4733 17th Avenue South,  
Minneapolis, MN 55407 (US). FABIAN, Willa, M.; 7018  
Tupa Circle, Edina, MN 55439 (US). CLARK, Larry,

For two-letter codes and other abbreviations, refer to the "Guid-  
ance Notes on Codes and Abbreviations" appearing at the begin-  
ning of each regular issue of the PCT Gazette.

(54) Title: RESPONSIVE MANUFACTURING AND INVENTORY CONTROL

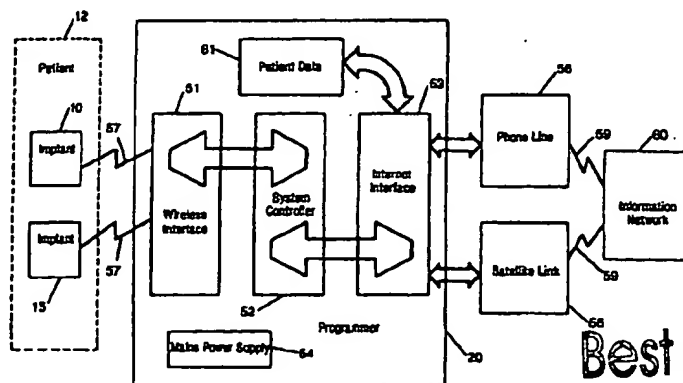

Best Available Copy

(57) Abstract: A medical device production and supply information management system synchronous with manufacturing, planning and scheduling, product consumption forecast, and component purchase to enable just-in-time inventory control at the manufacturing facility, vendor stocks, material/product tracking, distribution and shipping management to thereby reduce inventory at all points in the product manufacturing, distribution/delivery chain. The system is implemented using a preferably Web enabled information network and data communications with a programmer. The programmer provides access to product information, specification and related data for implanted medical devices from which build-to-order and build-to-replenish commands are issued to the manufacturing center. The system is interactive within the consumption management system that is integrally and seamlessly connected with patients, hospitals, sales offices and related information hubs including manufacturing facilities. The invention enables management of inventory levels of medical devices through the interactive information management system by accurately accounting for inventory stored in sales offices, distributors and sales representatives, as well as implanting institutions to ensure that all centers have appropriate and adequate stock that is replaced on just-in-time basis under the build-to-replenish scheme.

15/9/1 (Item 1 from file: 2)  
DIALOG(R) File 2:INSPEC  
(c) 2004 Institution of Electrical Engineers. All rts. reserv.

5837535 INSPEC Abstract Number: B9804-7230-005, C9804-7410D-003

Title: **Primary response of high-aspect-ratio thermoresistive sensors**  
Author(s): Majlese, H.R.; Mitchell, D.L.; Bhattacharya, P.K.; Singh, A.; Anderson, J.A.

Author Affiliation: Southern Univ., Baton Rouge, LA, USA  
Journal: Proceedings of the SPIE - The International Society for Optical Engineering Conference Title: Proc. SPIE - Int. Soc. Opt. Eng. (USA)  
vol.3068 p.388-94

Publisher: SPIE-Int. Soc. Opt. Eng.,  
Publication Date: 1997 Country of Publication: USA  
CODEN: PSISDG ISSN: 0277-786X  
SICI: 0277-786X(1997)3068L:388:PRHA;1-J  
Material Identity Number: C574-97213  
U.S. Copyright Clearance Center Code: 0277-786X/97/\$10.00  
Conference Title: Signal Processing, Sensor Fusion, and Target Recognition VI

Conference Sponsor: SPIE  
Conference Date: 21-24 April 1997 Conference Location: Orlando, FL, USA

Language: English Document Type: Conference Paper (PA); Journal Paper (JP)

Treatment: Applications (A); Practical (P)

Abstract: There is a growing need for sensors in monitoring performance in modern quality products such as in electronics to monitor heat build up, substrate delaminations, and thermal runaway. In processing instruments, intelligent sensors are needed to measure deposited layer thickness and resistivities for process control, and in environmental electrical enclosures, they are used for climate monitoring and control. A yaw sensor for skid prevention utilizes very fine moveable components, and an automobile engine controller blends a microprocessor and sensor on the same chip. An active-pixel image sensor is integrated with a digital readout circuit to perform most of the functions in a video camera. Magnetostrictive transducers sense and damp vibrations. Improved acoustic sensors are used in flow detection of air and other fluids, even at subsonic speeds. Optoelectronic sensor systems are being developed for installation on rocket engines to monitor exhaust gases for signs of wear in the engines. With new freon-free coolants being available the problems of A/C system corrosion have gone up in automobiles and need to be monitored more frequently. Defense cutbacks compel the storage of hardware in safe-custody for an indeterminate period of time, and this makes monitoring more essential. Just-in-time customized manufacturing in modern industries also needs dramatic adjustment in productivity of various selected items, leaving some manufacturing equipment idle for a long time, and therefore, it will be prone to more corrosion, and corrosion sensors are needed. In the medical device industry, development of implantable medical devices using both potentiometric and amperometric determination of parameters has, until now, been used with insufficient micro miniaturization, and thus, requires surgical implantation. In many applications, high-aspect-ratio devices, made possible by the use of synchrotron radiation lithography, allow more useful devices to be produced. High-aspect-ratio sensors will permit industries and various other users to attain more accurate measurements of physical properties and chemical compositions in many systems. Considerable engineering research has recently been focused on this type of fabrication effect. This paper looks at a high-aspect-ratio sensor bus thermorestrictive device with increased aspect-ratio of the interconnects to the device, using unique simulation software resources. (5 Refs)

Subfile: B C

Descriptors: circuit analysis computing; digital simulation; electrical conductivity; SPICE; temperature sensors

Identifiers: high-aspect-ratio thermoresistive sensors; performance monitoring; substrate delaminations; thermal runaway; Pspice program ;

Best Available Copy

intelligent sensors; deposited layer thickness; resistivities; process control; environmental electrical enclosures; climate monitoring; climate control; yaw sensor; skid prevention; automobile engine controller; microprocessor chip; active-pixel image sensor; digital readout circuit; magnetostrictive transducers; just-in-time customized manufacturing; implantable medical devices; synchrotron radiation lithography; simulation software

Class Codes: B7230 (Sensing devices and transducers); B7320R (Thermal variables measurement); B1130B (Computer-aided circuit analysis and design); C7410D (Electronic engineering computing); C6185 (Simulation techniques)

Copyright 1998, IEE

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
9 August 2001 (09.08.2001)

PCT

(10) International Publication Number  
**WO 01/56654 A1**

(51) International Patent Classification<sup>7</sup>: A61N 1/372,  
A61B 5/00, G06F 17/60

G.; 3720 Wellington Court, Plymouth, MN 55441 (US).  
THOMPSON, David, L.; 14171 Alder Street Northwest,  
Andover, MN 55304 (US).

(21) International Application Number: PCT/US01/03417

(22) International Filing Date: 2 February 2001 (02.02.2001)

(74) Agents: WOLDE-MICHAEL, Girma et al.; Medtronic,  
Inc., MS301, 7000 Central Avenue NE, Minneapolis, MN  
55432 (US).

(25) Filing Language: English

(81) Designated States (national): CA, JP.

(26) Publication Language: English

(84) Designated States (regional): European patent (AT, BE,  
CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC,  
NL, PT, SE, TR).

(30) Priority Data:  
60/180,289 4 February 2000 (04.02.2000) US


(71) Applicant: MEDTRONIC, INC. [US/US]; 7000 Central  
Avenue NE, Minneapolis, MN 55432 (US).

Published:  
— with international search report  
— before the expiration of the time limit for amending the  
claims and to be republished in the event of receipt of  
amendments

(72) Inventors: MCMENIMEN, James, L.; 935 East LaJol-  
lia Drive, Tempe, AZ 85282 (US). CAMPBELL, Christo-  
pher, J.; 707 Heron Circle North, Oakdale, MN 55128  
(US). RUBLE, Barbara, K.; 4733 17th Avenue South,  
Minneapolis, MN 55407 (US). FABIAN, Willa, M.; 7018  
Tupa Circle, Edina, MN 55439 (US). CLARK, Larry,

For two-letter codes and other abbreviations, refer to the "Guid-  
ance Notes on Codes and Abbreviations" appearing at the begin-  
ning of each regular issue of the PCT Gazette.

(54) Title: RESPONSIVE MANUFACTURING AND INVENTORY CONTROL

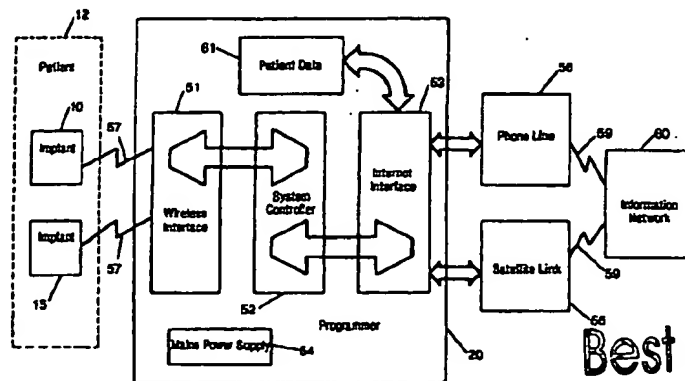

Best Available Copy

(57) Abstract: A medical device production and supply information management system synchronous with manufacturing, planning and scheduling, product consumption forecast, and component purchase to enable just-in-time inventory control at the manufacturing facility, vendor stocks, material/product tracking, distribution and shipping management to thereby reduce inventory at all points in the product manufacturing, distribution/delivery chain. The system is implemented using a preferably Web enabled information network and data communications with a programmer. The programmer provides access to product information, specification and related data for implanted medical devices from which build-to-order and build-to-replenish commands are issued to the manufacturing center. The system is interactive within the consumption management system that is integrally and seamlessly connected with patients, hospitals, sales offices and related information hubs including manufacturing facilities. The invention enables management of inventory levels of medical devices through the interactive information management system by accurately accounting for inventory stored in sales offices, distributors and sales representatives, as well as implanting institutions to ensure that all centers have appropriate and adequate stock that is replaced on just-in-time basis under the build-to-replenish scheme.

## RESPONSIVE MANUFACTURING AND INVENTORY CONTROL

### FIELD OF THE INVENTION

5           The present invention relates to systems and methods of manufacturing medical devices. Specifically, the invention relates to an interactive system in which a manufacturing computer server interacts with various data centers or hubs to collect enabling information for various build-to-order scenarios. The system is interactive with an information management system that is integrally and seamlessly connected with  
10       patients, hospitals, sales offices, and related information hubs. More specifically, the manufacturing and inventory control system of the present invention provides an automated and interactive system which derives manufacturing requirements, on a real-time basis, for replacing medical devices and components which have recently been consumed or implanted based on inputs from the various information hubs connected to a  
15       web-enabled information communication system.

### BACKGROUND OF THE INVENTION

          Over the years, many implantable devices have been developed to monitor medical conditions and deliver therapy to a patient. Such devices included electrical stimulation devices for stimulating body organs and tissue to evoke a response for enhancing a body  
20       function or to control pain, and drug delivery devices for releasing a drug bolus at a selected site. Other more passive implantable and wearable medical devices have been developed for monitoring a patient's condition.

          Chronically implanted cardiovascular devices for monitoring cardiovascular conditions and providing therapies for treating cardiac arrhythmias have vastly improved  
25       patients' quality of life as well as reduced mortality in patients susceptible to sudden death due to intractable, life threatening tachyarrhythmias.

          Such implanted devices can also process the patient's electrogram and any measured physiological conditions employed in the diagnosis and store the data, for subsequent telemetry out on interrogation by the external programmer. In general, the  
30       manner of communicating between the transceivers of the external programmer and the implanted device during programming and interrogating is referred to as telemetry.

The short range of conventional device telemetry is itself viewed as unduly limiting the communication of information over a long distance. In the medical monitoring field, longer range, continuously accessible telemetry has been sought and systems for doing so have been proposed. In U.S. Pat. No. 5,113,869, *Implantable Ambulatory Electrocardiogram Monitor* to Nappholz, et al, for example, an implanted ambulatory ECG patient monitor is described that is provided with longer range telemetry communication with a variety of external accessory devices to telemeter out alarm signals and ECG data and to receive programming signals. The high frequency RF signals are encoded, including the implanted device serial number, to ensure that the communication is realized only with the proper implanted device and that it is not misprogrammed.

A remote, external programmer and analyzer as well as a remote telephonic communicator are also described that may be used in addition to, or alternately to, the personal communicator alarm and/or the full disclosure recorder. The programmer and analyzer may operate at a distance to the implanted AECG monitor to perform programming and interrogation functions. The implanted AECG may automatically transmit a beacon signal to the programmer and analyzer to initiate an interrogation function to transmit data to the programmer and analyzer on detection of an arrhythmia or a malfunction of the implanted AECG monitor detected in a self-diagnostic test. Or by setting a timer in the personal communicator alarm, the implanted AECG monitor may be automatically interrogated at preset times of day to telemeter out accumulated data to the telephonic communicator or the full disclosure recorder. The remote telephonic communicator may be part of the external programmer and analyzer and is automatically triggered by the alarm or data transmission from the implanted AECG monitor to establish a telephonic communication link and transmit the accumulated data or alarm and associated data to a previously designated clinic or physician's office through a modem.

A similar hand-held interrogator for an implanted pacemaker-cardioverter-defibrillator device is disclosed in U.S. Pat. No. 5,336,245, *Storage Interrogation Apparatus for Cardiac Data*, issued to Adams and Kroll in 1994, wherein the data accumulated in a limited capacity memory implanted device is telemetered out to a larger capacity, external data recorder. The accumulated data is also forwarded to a clinic

employing an auto-dialer and FAX modem resident in a personal computer-based, programmer/interrogator.

U.S. Patent No. 5,752,976, *World wide patient location and data telemetry system for implantable medical devices*, issued to Duffin, et al, in May 1998, referenced herein in its totality, is instructive for the present invention. This patent describes a system for communicating patient device information to and from a medical device implanted in an ambulatory patient and with a remote medical support network comprising: an implanted device telemetry transceiver within the implanted medical device for communicating data and operating instructions to and from the medical device in a coded communication, the implanted device telemetry transceiver having a transceiving range extending outside the patient's body a predetermined distance sufficient to receive and transmit coded telemetry communications at a distance from the patient's body; and an external patient communications control device adapted to be located in relation to the patient within the device transceiving range having a system controller for facilitating communications, an implant wireless interface including a control device telemetry transceiver for receiving and transmitting coded communications between the system controller and the implant device telemetry transceiver, a global positioning system coupled to said system controller for providing positioning data identifying the global position of the patient to the system controller; communications means for communicating with the remote medical support network; and communications network interface means coupled to the system controller and the communications means for selectively enabling the communications means for transmitting the positioning data to the medical support network and for selectively receiving commands from the medical support network. The medical support staff may initiate data/programming communications with the implanted medical device.

U.S. Patents No. 5,891,180, *Interrogation of an Implantable Medical Device Using Audible Sound Communication*, to Greeninger et al, and No. 6,082,367, *Audible Sound Communication from an Implantable Medical Device*, to Greeninger and Thompson, both hereby incorporated by reference, are instructive on how data may be interrogated and telemetered out of the implanted device.

One of the issues unresolved by the '976 patent is the question of how to use this system to ensure that the implanting institution has an adequate inventory of implanted

devices. If the information about inventory status at the implanting institution, such as the implantation of a medical device (a reduction in inventory) could be telemetered to the manufacturing site, the manufacturer could then build an identical device to replace the recently implanted device—a process called “build-to-order”.

5           Build-to-Order manufacturing and control systems are well known to those familiar with the art. Such systems were pioneered by Dell USA, when the company's founder, as far back as 1985, began to manufacture and assemble computers to meet the needs of the user customer. This method of manufacturing and delivery of the product has been further enhanced by allowing potential customers to specify the exact type of desktop  
10           or laptop computer s/he wishes to purchase. Overhead, in the form of an outlet store with its accompanying sales personnel and incremental costs, are non-existent. As a result, Dell USA is able to consistently provide quality products at consistently lower costs, as compared to its competition. Dell USA holds well over 200 patents, many of which relate directly to the design and implementation of its build-to-order process. To mention but  
15           two such patents, we may cite U.S. Patent Nos. 5,894,571 *Process for Configuring Software in a Build-to-Order Computer System*, issued to O'Connor, and 5,995,757 *Software Installation and Testing for a Build-to-Order Computer System*, both hereby referenced in their totality.

          Another model that may be cited comes from IBM that holds U.S. Patent No.  
20           6,078,900 in June, 2000, *Method for Estimating Stock Levels in Production-Distribution Networks with Inventory Control*, issued to Amberg et al., also referenced herein in its totality. That invention provides computer software for business management and a computer implemented method for estimating stock levels in production-distribution networks with inventory control.

25           There are many similarities between the computer industry and the medical device industry. Thus, it should be possible to adapt and improve upon these well-known build-to-order systems and methods to fit the needs of the medical device industry.

          Medical device industries are growing at a rapid rate with a corresponding rapid growth and change in their production processes. At present, the distribution of these  
30           products requires multiple stockholding points. One of the great challenges in the medical device environment is a company's ability to meet end-customer demand for an adequate



inventory to provide immediate availability for medical devices for which the need cannot be predicted in advance. Consuming (implanting) devices prior to the expiration of a device's shelf life and managing the transition to newly approved devices (e.g., by the FDA) pose additional challenges.

5           If inventories are managed successfully, rewards can be tremendous. However, the penalty for keeping too little stock or failure to replace stock in a hospital goes beyond the cost of foregone revenue for both the manufacturer and the hospital. It includes the potential for loss of life because the individual required medical device is not available. The penalty for keeping too much stock in inventory, on the other hand, includes the cost  
10           of financing a large inventory thereby reducing profit margins to those medical institutions. Further, the need to implant products before obsolescence and managing a smooth transition into new products pose various strategic and manufacturing challenges. Furthermore, consuming (implanting) devices prior to the expiration of a device's shelf life and managing the transition to newly approved devices (e.g., by the FDA) pose  
15           additional challenges.

          The initial stocking of inventory, as currently practiced, involves the manufacturer's representative and a person at the institution who is intimately familiar with the usage of medical devices and the number of devices used by the medical institution, often the hospital administrator. Assuming the institution has purchased a  
20           certain number of devices, the representative ensures that the institution has a certain number of these devices on the "shelves." The type of device and their number will reflect the nature and content of the contract governing the business relations, between the institution and the manufacturer and is usually based on expected, rather than actual, usage. Thus, there may be a distribution between basic, advanced, and more advanced  
25           technology, again conforming to the nature of the contract that governs the sale of such devices.

          The manufacturer's representative maintains that initial inventory. If, however, and for one reason or another, the physician implanter has a greater number of patients who require the implantation of a medical device of one sort or another, the inventory of  
30           specific medical devices may become depleted. The situation often arises where the depletion of devices is not noticed until the physician requests a device to match the needs

of the patient to be implanted the next day, or later in the day on which the request is made. What is to be done then? Usually a call is made to the manufacturer's local business office that may or may not have the exact model on hand. If so, someone has to bring it to the institution. This may involve many miles depending on the location of the business office relative to the medical institution. If this device is not available at the local business office, a call will be made to the manufacturer's central office or to the manufacturing facility. In such cases and even when Herculean efforts take place, the device will not usually arrive at the institution in time for the original scheduled implant. Often the implant must be postponed for several days. This is the primary issue that the present invention addresses.

A secondary issue that must be addressed occurs during those times when the device manufacturer is introducing a new product. The manufacturing facility must have on hand a rather large number of newer devices which the physicians and institutions will request for use upon approval for implant is received from an approving agency such as the FDA in the U.S.A. and other such agencies in Europe and Japan. Yet, until approval is given, none of the newer devices may be implanted. Only those that were previously approved may be implanted. If the approval is delayed for one reason or another, the manufacturer must maintain two inventories, one of the older and one of the newer product lines. In such cases, when approval is finally granted and because the physicians usually wish to make use of the newer technology, the manufacturer must usually retrieve the older product inventory and dispose of it in some way or other, usually at an economic loss to the manufacturer which, in turn, can bring about a subsequent increase in cost to the government, insurance payer, or patient.

The key challenge that the medical device industry must face is to determine where and in what quantities to hold safety stock in the network so as to protect against uncertainties, and to ensure that target customer service levels are met. Aggressive service requires significant inventory planning. Today, the determination of inventory levels is localized and often ad hoc, and not based on an analysis of optimal levels and deployment. As a result, the business impact, in terms of the trade-off between inventory investment and customer serviceability or delinquency, is far from optimal.

Determining the optimal inventory levels in individual medical institutions is extremely difficult, and few real-world inventory management systems have the capability to accurately predict target stock levels. The difficulty of the problem arises from the fact that the quantity of safety stock held at one stocking location, and the policy determining replenishment of inventory at that location, will affect other stockholding locations in the network. A system is needed that accurately represents the interdependencies of all links in a production-distribution network, and allows the manufacturer of medical devices to fill the institution's inventory on an automatic basis whenever that inventory is depleted by even one device as it is used.

Modern medical devices contain highly sophisticated hardware and software components that require specialized manufacturing processes. Further, these same devices require replacement on the shelves of a hospital on a timely basis when a unit in inventory is implanted in a patient. Hospitals, physicians, and other patient-care systems operate in a highly constrained economic environment. Inventory control is one way to reduce costs within these medical systems. Thus, a medical device manufacturing system that is interactive with and responsive to this environment is highly desirable. This is especially true if such a system can minimize the need for maintaining a large inventory of these medical devices, while sustaining the institution's ability to deliver efficient and effective medical care.

What is needed is a system that has the following goals: build products to refill the medical institution's inventory order, automatic replenishment of stock in days, and track manufacturing and product information in order to effectively service customers.

#### SUMMARY OF THE INVENTION

This invention builds on the previously filed application 09/430,208, *Automatic Invoice Upon Pacemaker Implant* by Linberg on Oct. 29, 1999, hereby referenced in its totality, which describes an auto-invoicing system. With the data acquired with this system, the present invention makes it possible to manage inventory levels of products implanted ("consumed"). On the one hand, this invention manages inventory at any place products are stored, such as in sales offices, with individual sales representatives, and ultimately at the implanting institution to ensure that the appropriate and adequate stock is quickly replaced on just-in-time basis always available. These devices include—but are

not limited to—implantable pacemakers, cardioverter-defibrillators, neurological stimulators, leads, drug delivery systems, lead adapters, lead repair kits, etc. On the other hand, this invention may be used to control and manage manufacturing planning and scheduling, forecasting product consumption, purchasing device components, inventory control at the manufacturing facility, vendor management, material tracking, capacity  
5 planning, distribution and shipping of finished product, etc.

The required data, for example that a specific device with its associated lead(s) , has been implanted may be transferred by the programmer to the Information Network, described in the '976 patent. These data may be downloaded on a real time basis or on a  
10 daily basis, usually at night. The Information Network will then summarize these data on a daily basis and issue a built order to replenish the stock that was "consumed" at implant for the specific implanting institution. Specifically, the device type, model number, serial number, name of the implanting physician, the name of the sales representative, the name of the implanting institution are automatically downloaded to the Information Network  
15 through the programmer, as substantially described in U.S. Patent No. 5,345,362 and Des. 358,583 by Winkler, both of which are incorporated by reference in their entirety. These data, when received, would in turn automatically initiate a "build-to-order" replenishment to match and replace the device(s) implanted at that institution.

Although the intention of this process is to have a very quick turnaround time, e.g.,  
20 a total of two days from notification of implant, building the product in an automated assembly line, and delivery of the product, it is also possible that the status of the product build could be made available to all interested parties (purchase agent, physician, hospital administrator, sales rep, etc.) on an ongoing basis. Other benefits would include substantial cost savings in manufacturing, reduced product cycle times, reduced  
25 obsolescence, reduced inventories at all points in the product delivery chain, and so on. This process will minimize inventory issues for the account, as well as for the manufacturer. In addition it will make it easier to ramp up for the introduction of a new product while, at the same time ramping down the build of the old product. "Phase out" should be much simpler and quicker. With the attainment of these benefits, the costs to the  
30 implanting institution can also be controlled and reduced significantly.

Using this invention, the implanting institution's inventory is automatically managed. For example, the Information Network could recommend an alternative device to replace a "used" device. This might occur when products are being phased in or phased out or when a new product is approved for implantation by the specific approving agency in a geographic area. Automatic notifications, based on local regulatory controls, could be placed on labels or within the shipping package so that restrictions on the product's usage, warnings, alerts, etc. could be communicated and implemented. Additionally, the institution and/or implanting physician will be able to monitor the status of the build process, the expected completion, and the status of shipping and scheduled delivery, all of which is commonly known and expected in the shipping industry (i.e., Federal Express or UPS tracking systems).

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of a body-implantable device system in accordance with the present invention, including a hermetically sealed device implanted in a patient and an external programming unit.

FIG. 2 is a perspective view of the external programming unit of FIG. 1.

FIG. 3 is a block diagram of a system in which the invention is practiced for a patient receiving an implantable medical device, in communication with a programmer, which is in communication with the Information Network employing Internet telecommunication and/or satellite linkage.

FIG. 4 is a block diagram of the present invention describing the multiple steps that occur in the manufacturing facility from receipt of the order to shipment of the device to the implanting institution.

#### DETAILED DESCRIPTION OF THE DRAWINGS

The present invention uses the Global Communications and Monitoring System (GCMS) described in the '976 patent. This system provides a means for exchanging information with and exercising control over one or more medical devices implanted within the body of a patient employing the patient communications control device. The GCMS is intended to function no matter how geographically remote the patient may be relative to the monitoring site or medical support network. As such, then, during the implant procedure, with the patient in very close proximity to the programmer, there

should be no difficulty in establishing communications between the implanted device and the programmer. In this situation, the programmer determines location and details relevant to the device communicates those data via a cellular telephone system link or a satellite based telecommunications link if the patient is outside the range of a cellular link or subscribes only to the satellite-based link.

FIG. 1 is an illustration of an implantable medical device system adapted for use in accordance with the present invention. The medical device system shown in FIG. 1 includes an implantable device 10—a pacemaker for illustration purposes—that has been implanted in a patient 12. In accordance with conventional practice in the art, pacemaker 10 is housed within a hermetically sealed, biologically inert outer casing, which may itself be conductive so as to serve as an indifferent electrode in the pacemaker's pacing/sensing circuit. One or more pacemaker leads, collectively identified with reference numeral 14 in FIG. 1 are electrically coupled to pacemaker 10 in a conventional manner and extend into the patient's heart 16 via a vein 18. Disposed generally near the distal end of leads 14 are one or more exposed conductive electrodes for receiving electrical cardiac signals and/or for delivering electrical pacing stimuli to heart 16. As will be appreciated by those of ordinary skill in the art, leads 14 may be implanted with their distal end(s) situated in the atrium and/or ventricle of heart 16.

Although the present invention will be described herein in an embodiment which includes a pacemaker, those of ordinary skill in the art having the benefit of the present disclosure will appreciate that the present invention may be advantageously practiced in connection with numerous other types of implantable medical device systems, and indeed in any application in which it is desirable to provide a communication link between two physically separated components.

Also depicted in FIG. 1 is an external programming unit 20 for non-invasive communication with implanted device 10 via uplink and downlink communication channels, to be hereinafter described in further detail. Associated with programming unit 20 is a programming head 22, in accordance with conventional medical device programming systems, for facilitating two-way communication between implanted device 10 and programmer 20. In many known implantable device systems, a programming head such as that depicted in FIG. 1 is positioned on the patient's body over the implant site of

the device (usually within 2- to 3-inches of skin contact), such that one or more antennae within the head can send RF signals to, and receive RF signals from, an antenna disposed within the hermetic enclosure of the implanted device or disposed within the connector block of the device, in accordance with common practice in the art. In addition, programmer 20 is also equipped with a transceiver and/or modem to facilitate communication between programmer 20 and the Internet.

FIG. 2 is a perspective view of programming unit 20 in accordance with the presently disclosed invention. Internally, programmer 20 includes a processing unit (not shown in the Figure) that in accordance with the presently disclosed invention is a personal computer type motherboard, e.g., a computer motherboard including an Intel Pentium 3 microprocessor and related circuitry such as digital memory. The details of design and operation of the programmer's computer system will not be set forth in detail in the present disclosure, as it is believed that such details are well-known to those of ordinary skill in the art. In addition, there is a transceiver (not shown) that is used to communicate data wirelessly (telemetry) from the implanted device to an Information Network (see FIGs. 3 and 4). Alternatively, a modem and landlines may be used.

The FCC has adopted the following definition for describing wireless medical telemetry: "the measurement and recording of physiological parameters and other patient-related information via radiated bi- or unidirectional electromagnetic signals." Thus, in its broadest sense, telemetry can be defined as the art and science of conveying information from one location to another. With radio telemetry, radio signals are utilized to convey that information.

"Telemedicine" is the use of telecommunications and information technology to provide clinical care or data at a distance. The definition of "distance" may range from several yards, such as might occur within a clinic environment or hundreds of miles as occurs in transmission of such data between an implanting institution and an Information Network, as envisaged in the present invention. Wireless technology can be particularly beneficial because developing wireless networks may be faster and cheaper than building a landline infrastructure.

Medical telemetry equipment is increasingly relied upon in hospitals to improve health care and reduce costs. The number of pacemaker patients with chronic medical

conditions is rising due to the growth in the elderly population. For these reasons, the need for ensuring the availability of an adequate inventory of pacemakers within the implanting hospital is vital and this need can be fulfilled with medical telemetry equipment such as that used in the programmer depicted in FIG. 2

5 Referring to FIG. 2, programmer 20 comprises an outer housing 60, which is preferably made of thermal plastic or another suitably rugged yet relatively lightweight material. A carrying handle, designated generally as 62 in FIG. 2, is integrally formed into the front of housing 60. With handle 62, programmer 20 can be carried like a briefcase.

An articulating display screen 64 is disposed on the upper surface of housing 60.

10 Display screen 64 folds down into a closed position (not shown) when programmer 20 is not in use, thereby reducing the size of programmer 20 and protecting the display surface of display 64 during transportation and storage thereof. Stylus 24 is used for data entry and/or control of programmer 20.

15 A floppy disk drive is disposed within housing 60 and is accessible via a disk insertion slot (not shown). A hard disk drive is also disposed within housing 60, and it is contemplated that a hard disk drive activity indicator, (e.g., an LED, not shown) could be provided to give a visible indication of hard disk activation.

As would be appreciated by those of ordinary skill in the art, it is often desirable to provide a means for determining the status of the patient's conduction system. Normally, programmer 20 is equipped with external ECG leads. These leads may be rendered  
20 redundant if the implanted device is equipped with a "subcutaneous electrode array" as described in the filed application 09/749,169, *Leadless Fully Automatic Pacemaker Follow-Up*, by Combs et al., filed December 12, 2000.

Programmer 20 is equipped with an internal printer (not shown) so that a hard copy  
25 of a patient's ECG or of graphics displayed on the programmer's display screen 64 can be generated. Several types of printers, such as the AR-100 printer available from General Scanning Co., are known and commercially available.

30 In the perspective view of FIG. 2, programmer 20 is shown with articulating display screen 64 having been lifted up into one of a plurality of possible open positions such that the display area thereof is visible to a user situated in front of programmer 20. Articulating display screen is preferably of the LCD or electro-luminescent type, characterized by



being relatively thin as compared, for example, a cathode ray tube (CRT) or the like.

As would be appreciated by those of ordinary skill in the art, display screen 64 is operatively coupled to the computer circuitry disposed within housing 60 and is adapted to provide a visual display of graphics and/or data under control of the internal computer.

5 Programmer 20 described herein with reference to FIG. 2 is described in more detail in the previously cited U.S. Pat. No. 5,345,362. The Medtronic Model 9790 programmer is the implantable device-programming unit with which the present invention may be advantageously practiced.

10 FIG. 3 is a block diagram of a system in which the invention is practiced. The major components of the system include at least one implanted medical device patient 12, programmer 20, and Information Network 60. Patient 12 may have multiple implants, for example, an implanted bradycardia type pacemaker 10 with and an implanted ICD 15 that has just been implanted. ICD 15, preferably communicates through RF link 57 to the programmer, specifically to wireless interface 51. Data, such as factory-programmed  
15 parameters and so on, are forwarded to system controller 52. Under a physician's direction/prescription, these parameters may be altered and downloaded from system controller 52 to ICD 15 via RF wireless interface 51.

Continuing with FIG. 3 and more to the point of its relation to the present invention, we see that the same data as well as the device's model number, serial number,  
20 date of implant, and so on are conveyed to system interface 53. At this juncture, the data may be stored (in patient data memory 61) or transmitted/telemetered immediately. The time of transmission is dependent on whether the programmer is or is not connected to phone link 56 or satellite link 55 at the time of implant. Assuming that one of these connections is made at some time during the day, the data from patient data 61 and  
25 Internet interface 53 is uplinked to the Internet via phone line modem connection 56 and phone line 59 or telemetric satellite link 55 using data encryption technology for a secure transmission as substantially described in filed application No. 09/431/881, *Method and Apparatus to Secure Data Transfer from Medical Device Systems*, filed November 2, 1999 by Nichols and incorporated herein by reference. Upon reaching Information Network 60,  
30 these data are incorporated into the data file containing the complete information relating to the implanting institution, for billing purposes and other uses. These same data are also

forwarded to that portion of the network computer related to new build orders for manufacturing, which relates to FIG. 4.

Turning our attention now to FIG. 4, we see the various steps used during the manufacturing process to ensure that the recently implanted ICD (using the example mentioned above) is replaced as quickly as possible. Once an implant has taken place at a particular institution the data is available to the Information Network 60 (see FIG. 3), that same network, which is constantly monitoring the "build-to-order" status 72. The network periodically determines whether a device needs to be built 70 for this particular institution. If No, then it continues to monitor for an implant. If Yes, then the implant data is downloaded to the manufacturing database 74. This includes all pertinent data relative to the implanted device. Specifically, these data will include the device type, model number, serial number, name of the implanting physician, the name of the sales representative, and the name of the implanting institution. These data, when received, will automatically initiate a "build-to-order" replenishment to match and replace the standard device(s) implanted at that institution.

Once the order is made, a comparison is made to assess whether the build will meet the planned inventory 76. In addition, the manufacturing database will determine whether all components required to complete the build are available 78 at the factory site located nearest to the implanting institution. If components are available, that factory site is selected and scheduled to complete the build 80. If components are not available, the manufacturing database issues an automatic component supplier order 94. The required components are noted and shipped by the supplier(s) 92 to the manufacturing site.

Initiating build 82 with available components or those delivered from the supplier results in building and assembly of the "standard" device, which will replace the implanted device in the inventory of the implanting institution. The implantable device is tested at various stages in the manufacturing process 84 and will undergo final testing prior to packaging 86 and sterilization. Finally, the device is shipped 88 to the implanting institution 90 for restocking in their inventory.

During this whole process, the purchasing agent and/or hospital administrator is able to discern exactly the stage that the device being manufactured has reached. Such information will be available on the Information Network that is accessed via the Internet

96. This same access to the Information Network is also available to the sales representative who is able to monitor the progress of the build and report to the implanting institution, if that institution is unable to access the Information Network—for whatever reason.

5           As previously mentioned, the goal for this Responsive Manufacturing and Inventory Control system is to deliver a replacement device within two working days of receipt of the information that a device has been implanted and must be replaced.

10           The preceding specific embodiments are therefore to be understood as illustrative of the many ways in which the principles of the invention may be practiced. It is to be understood, therefore, that other expedients known to those of skill in the art or disclosed herein may be employed without departing from the invention or the scope of the appended claims.

15           In the following claims, means-plus-function clauses are intended to cover the structures described herein as performing the recited function and not only structural equivalents but also equivalent structures. For example, although a nail and a screw may not be structural equivalents in that a nail employs a cylindrical surface to secure wooden parts together, whereas a screw employs a helical surface, in the environment of fastening wooden parts, a nail and a screw are equivalent structures.

20           It is therefore to be understood, that within the scope of the appended claims, the invention may be practiced otherwise than as specifically described without actually departing from the spirit and scope of the present invention.

**What is claimed is:**

1. A medical device manufacturing and supply information management system comprising:

a Web-enabled information network;

a programmer; and

at least one implanted medical device, deployed from a known source, said Web-enabled information network being in bi-directional data communications scheme with the programmer, and the programmer being in data communication with said implanted medical device.

2. The system of claim 1 wherein said Web-enabled information network implements a Global Communications and Monitoring system (GCMS).

3. The system of claim 1 wherein said Web-enabled information network includes one of a satellite based telecommunications link and a cellular link.

4. The system of claim 1 wherein said programmer is implemented to interface between the medical device and the Web-enabled information network via the bi-directional data communications scheme to store manufacturing information in addition to information about the at least one implanted medical device.

5. The system of claim 1 wherein said at least one implanted medical device includes one of a new implant or an old implant needing an upgrade.

6. The system of claim 1 wherein said known source includes at least one of a manufacturing center, hospital, sales office, distributor having data communications with the Web-enabled information network.

7. A medical device inventory and production control system synchronous with various phases of product manufacturing for standard, customized and newly approved, modified/redesigned devices and to stock various consumption hubs including hospitals,

sales offices, distributors and sales representatives on a just-in-time basis under a build to order and build to replenish production scheme, the system comprising:

a Web-enabled information network being in data communications with manufacturing, shipping/delivery and the various consumption hubs; and

5 at least one programmer being in a bi-directional communications link with the Web-enabled information network; and

at least one device implanted in a patient taken out of one of the consumption hubs, and having a wireless communication with the programmer to thereby route device information to the Web-enabled information network.

10

8. A method for managing medical device inventory and production to coordinate and maintain a just-in-time inventory on a build-to-order production scheme wherein a manufacturing process and sales/distribution hubs are synchronized to track the medical device at all points in the product manufacture, sale, delivery and implantation chain, the method comprising:

15

providing a Web-enabled information network having bi-directional data communications with the hubs;

maintaining an inventory of the medical devices at the hubs and at a manufacturing facility;

20

updating a hub's inventory when a medical device is consumed by implementing a build-to-order and build-to-replenish scheme; and

maintaining device identity and associated patient information via a programmer interface.

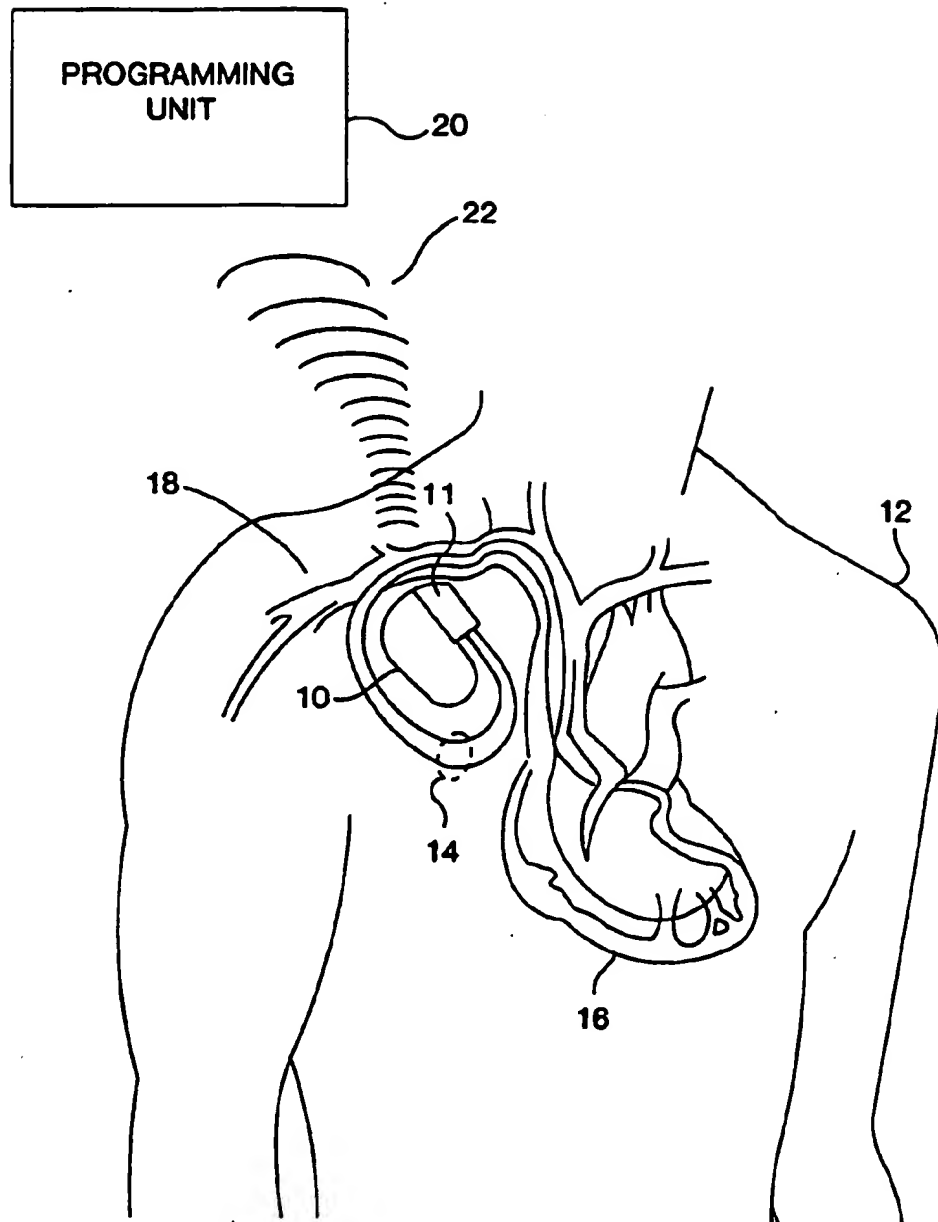


FIG. 1

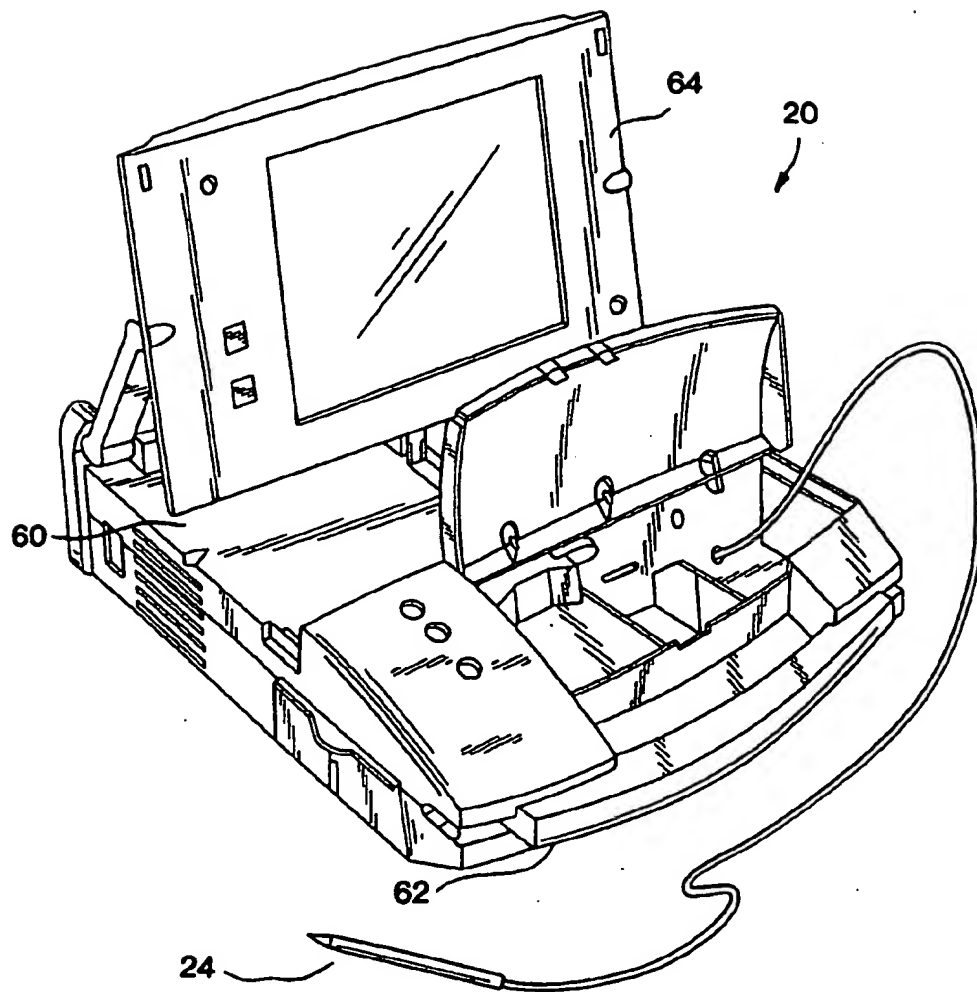


FIG. 2

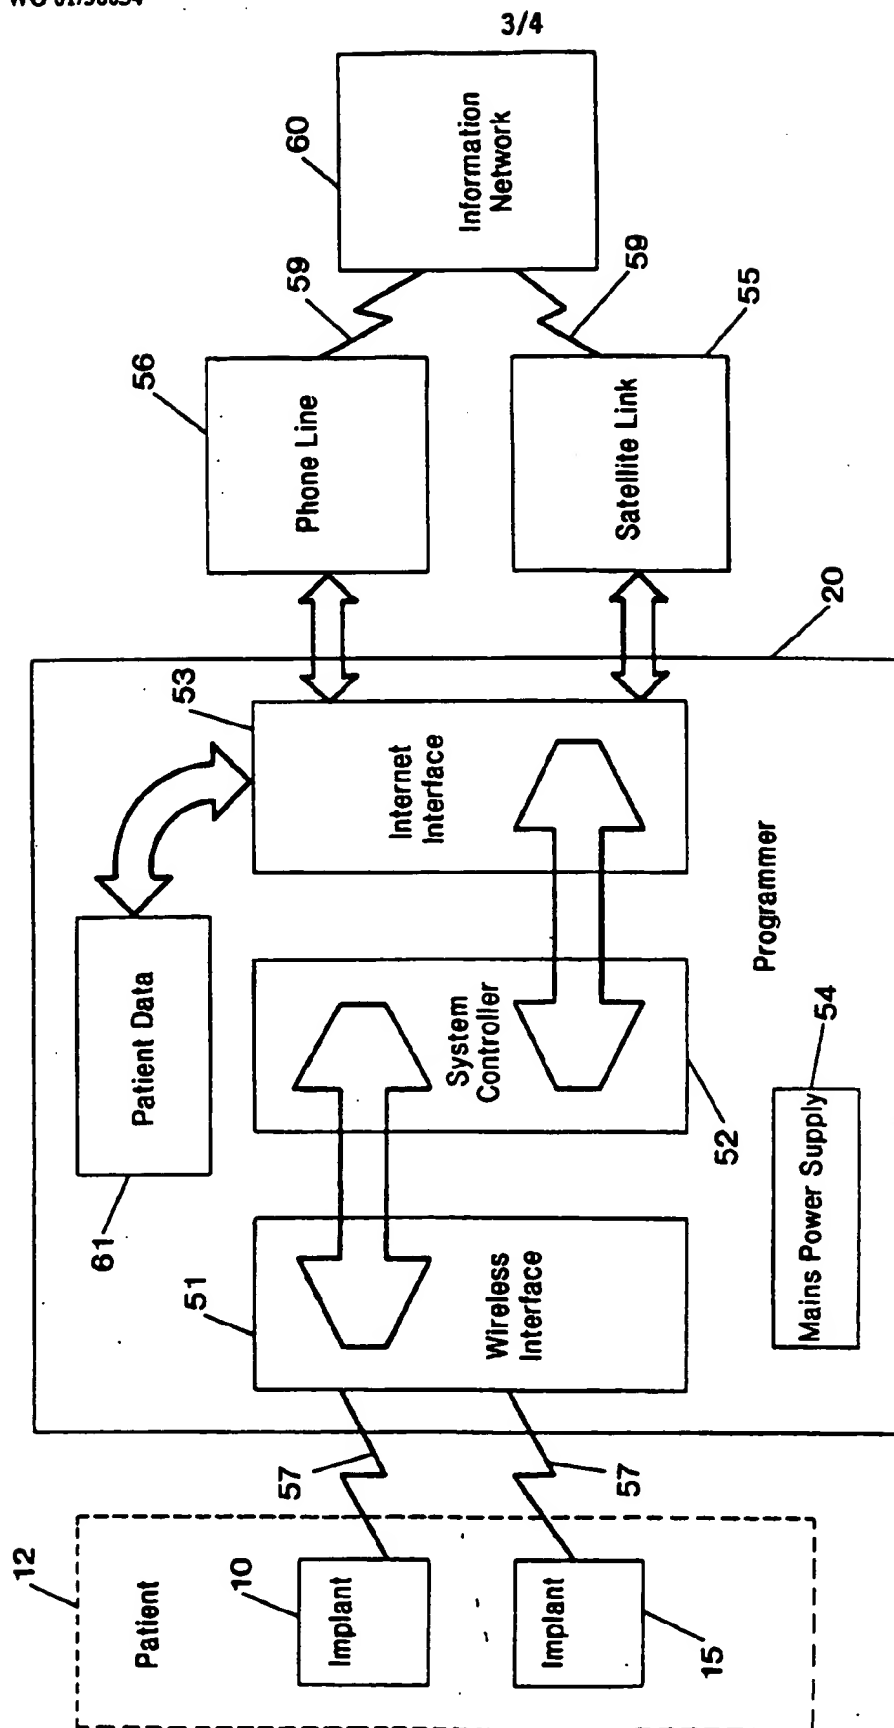


FIG. 3



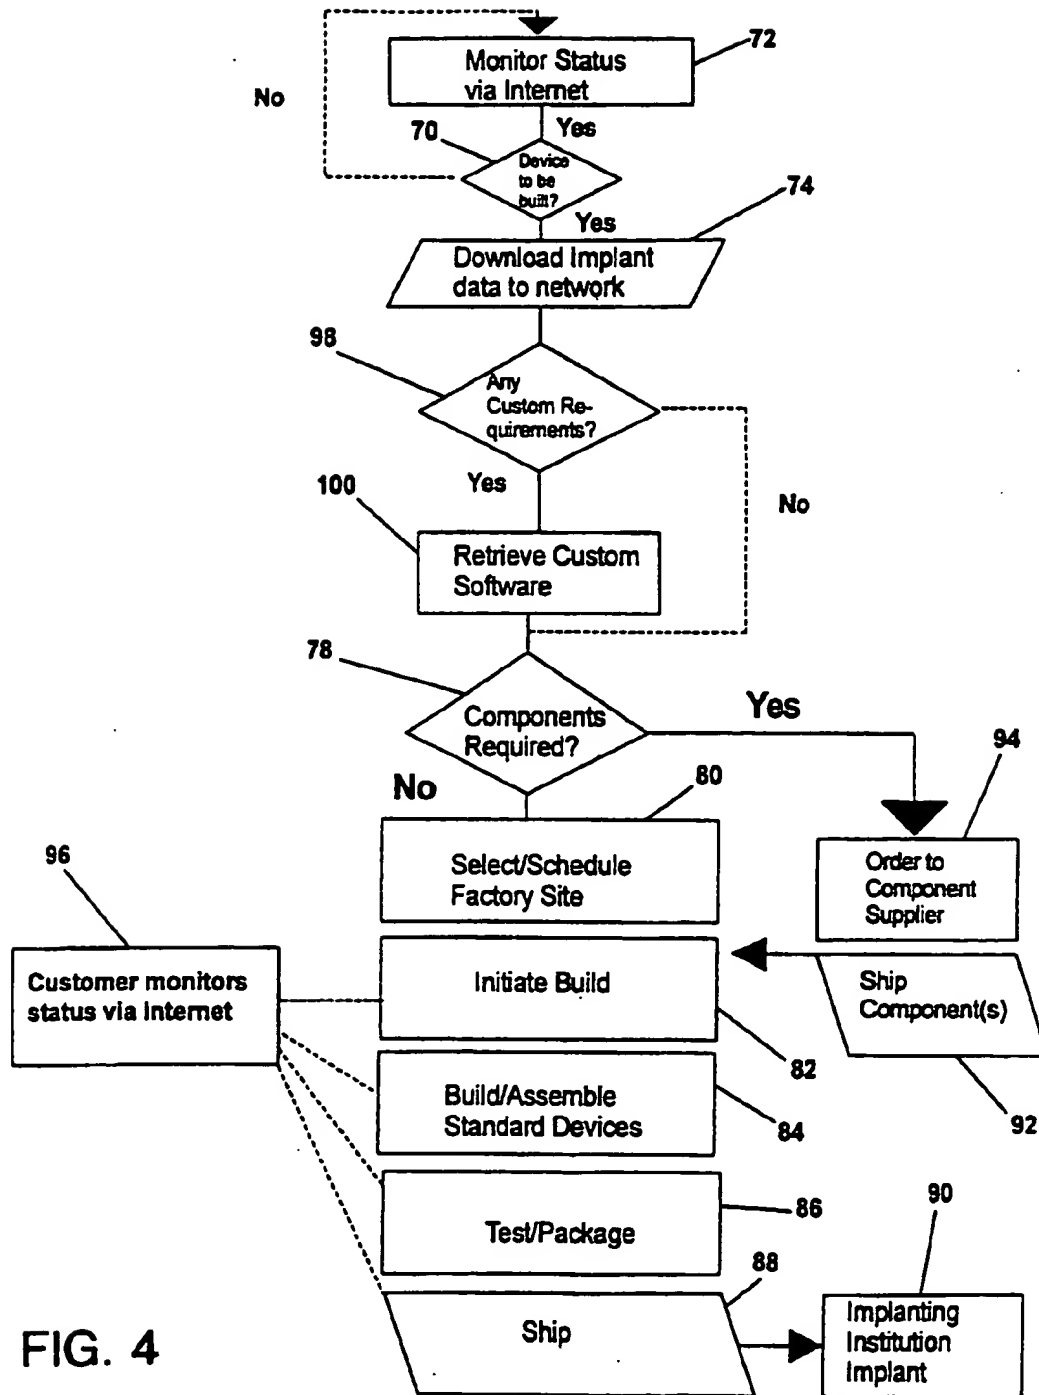


FIG. 4

# INTERNATIONAL SEARCH REPORT

Int. Application No.  
PCT/US 01/03417

**A. CLASSIFICATION OF SUBJECT MATTER**  
IPC 7 A61N1/372 A61B5/00 G06F17/60

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
IPC 7 A61N A61B G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, INSPEC

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 752 976 A (DUFFIN EDWIN G ET AL) 19 May 1998 (1998-05-19) column 4, line 35 -column 5, line 53	1-3,5-8
A	US 5 884 300 A (BROCKMAN RICHARD) 16 March 1999 (1999-03-16) column 2, line 15 -column 3, line 45; figure 2	1,7,8
A	US 5 434 775 A (KUSSWURM DANIEL C ET AL) 18 July 1995 (1995-07-18) column 1, line 24 -column 3, line 49	7,8
A	US 5 855 609 A (KNAPP TERRY R) 5 January 1999 (1999-01-05) column 6, line 38-67	1,6-8
	--- -/-- ---	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

\* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- \*G\* document member of the same patent family

Date of the actual completion of the international search

11 June 2001

Date of mailing of the international search report

22/06/2001

Name and mailing address of the ISA

European Patent Office, P.B. 5816 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel (+31-70) 340-2040, Tx 31 651 epo nl,  
Fax (+31-70) 340-3018

Authorized officer

Grossmann, C.

# INTERNATIONAL SEARCH REPORT

Int. Patent Application No  
PCT/US 01/03417

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 894 571 A (O'CONNOR CLINT H) 13 April 1999 (1999-04-13) cited in the application the whole document ---	1,7,8
A	WO 93 08872 A (MEDTRONIC INC) 13 May 1993 (1993-05-13) page 5, line 26 -page 6, line 15 -----	1,7,8

# INTERNATIONAL SEARCH REPORT

Information on patent family members

Int. l. Application No

PCT/US 01/03417

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5752976 A	19-05-1998	AU 709767 B AU 6176996 A CA 2224520 A EP 0939662 A JP 11508165 T WO 9700708 A US 6083248 A	09-09-1999 22-01-1997 09-01-1997 08-09-1999 21-07-1999 09-01-1997 04-07-2000
US 5884300 A	16-03-1999	NONE	
US 5434775 A	18-07-1995	AU 686269 B AU 8097394 A CA 2152276 A EP 0685090 A JP 8508359 T WO 9512858 A	05-02-1998 23-05-1995 11-05-1995 06-12-1995 03-09-1996 11-05-1995
US 5855609 A	05-01-1999	US 5674288 A US 5300120 A AU 4840896 A WO 9622049 A US 5725578 A AU 671859 B AU 4998493 A BR 9306964 A CA 2142993 A EP 0657056 A JP 8507698 T WO 9406105 A US 5716407 A US 5977431 A AT 189375 T AU 674022 B AU 5003093 A BR 9306947 A CA 2142995 A DE 69327802 D DE 69327802 T EP 0703760 A JP 8501956 T WO 9404094 A	07-10-1997 05-04-1994 07-08-1996 25-07-1996 10-03-1998 12-09-1996 29-03-1994 12-01-1999 17-03-1994 14-06-1995 20-08-1996 17-03-1994 10-02-1998 02-11-1999 15-02-2000 05-12-1996 15-03-1994 12-01-1999 03-03-1994 09-03-2000 12-10-2000 03-04-1996 05-03-1996 03-03-1994
US 5894571 A	13-04-1999	NONE	
WO 9308872 A	13-05-1993	AU 2258292 A US 5360437 A	07-06-1993 01-11-1994